


TC160 and TC400P5+ Nurse Call Systems • Rev. 0 - 10/2021

Background

The enclosed NC404TS is pre-assembled with the monitor stand. The monitor stand will need to be removed and reassembled with the provided bracket and screws. Please follow the disassembly and re-assembly instructions below.

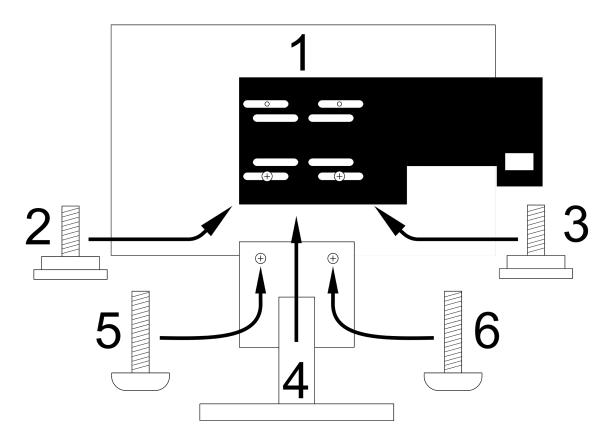

DISASSEMBLY

TOOLS NEEDED: PHILLIPS SCREWDRIVER

MONITOR WILL LIFT FREE AFTER REMOVING TWO SCREWS VISIBLE ON REAR REMOVE MONITOR FROM BASE REMOVE (AND RETAIN) TWO BLACK THREADED STANDOEES (ERONT OF MOUNTING PLACE

REMOVE (AND RETAIN) TWO BLACK THREADED STANDOFFS (FRONT OF MOUNTING PLATE)

RE-ASSEMBLY (SEQUENCE SHOWN ABOVE)

PLACE MONITOR SCREEN-DOWN ON SMOOTH, FLAT SURFACE ATTACH BRACKET (1) TO MONITOR AS SHOWN, USING BLACK THREADED STANDOFFS (2-3) ATTACH BASE (4) TO MONITOR+BRACKET USING TWO #4-14 SCREWS PROVIDED BY TEKTONE (5-6)

www.tektone.com

324 Industrial Park Road • Franklin, NC 28734 • tektone@tektone.com Phone: 828.524.9967 • Fax: 828.524.9968 • Sales: Choose option 2 • Tech Support: Choose option 3 TekTone's quality system is registered by DQS to the ISO 9001:2015 standard.